

Y039 Hand Operated Pressure Pump



Xi 'an Xinyi Instrument Technology Co. LTD

Application

1. The hand-operating pressure pump is a kind of pneumatic type hand-operating pressure source. It is designed to calibrate the pressure measuring instruments installed on the industrial working site and various pressure instruments in a control room. It can also provide the pressure source for any calibrating work in a factory. The hand operating pressure pump can calibrate pressure transmitters, pressure sensors and any kind of pressure instruments within the range of 0~ 230psi. The hand-operating pressure pump is portable and light. It has a wide range of temperature and ease of pumping up and operation.

It is designed with a fine adjuster and a vent-valve. Thus, the pressure regulation is harmonious with air.

The pump is easy for an operator to carry to the working site to directly calibrate pressure measuring instruments. Thus, the complicated process of removing and replacing on the working pipe or dismounting from a control room can be eliminated, resulting in an efficiency operation. The pump reached the advanced specifications of the same products made in foreign countries.

Construction and Working Principle

The pump (see the scheme) is comprised of a cylinder, a piston, a fine adjuster, a vent- -valve, a hand -grip and a fast speed connector. The hand-grip can be pressured and relieved by one hand repeatedly , thus causing the piston to reciprocate itself, with which the volume of the cylinder varies and output pressure develops up to 0~ 230 psi.

Technical Date

1. Operating pressure: 0~1. 6Mpa (0~2Mpa)

2. Operating temperature: - 20~ 50℃

3. Physical dimensions: 220x 110x 55mm


4. Weigh: 0.5kg

5. Spare parts:

a. Oring Y 039, 0000:04	1
b. Oring Y 039, 0000:18	1
c. Oring Y 039, 1000:02	1
d. Retaining ring 9 GB896	2
e. Retaining ring 3 GB896	2

Caustions

1. Use a pipe to connet both master pressure gauge and instrument to be calibrated.
2. While pumping up, please turn the vent- valve clockwise to leak tightness. While unloading, do it in opposite way.
3. When pressure instrument is being calibrated, each joint point should be airtight. After the calibration, make sure to relieve all the pressure prior to removing the instrument, if not it will be dangerous and the instrument will get damaged.

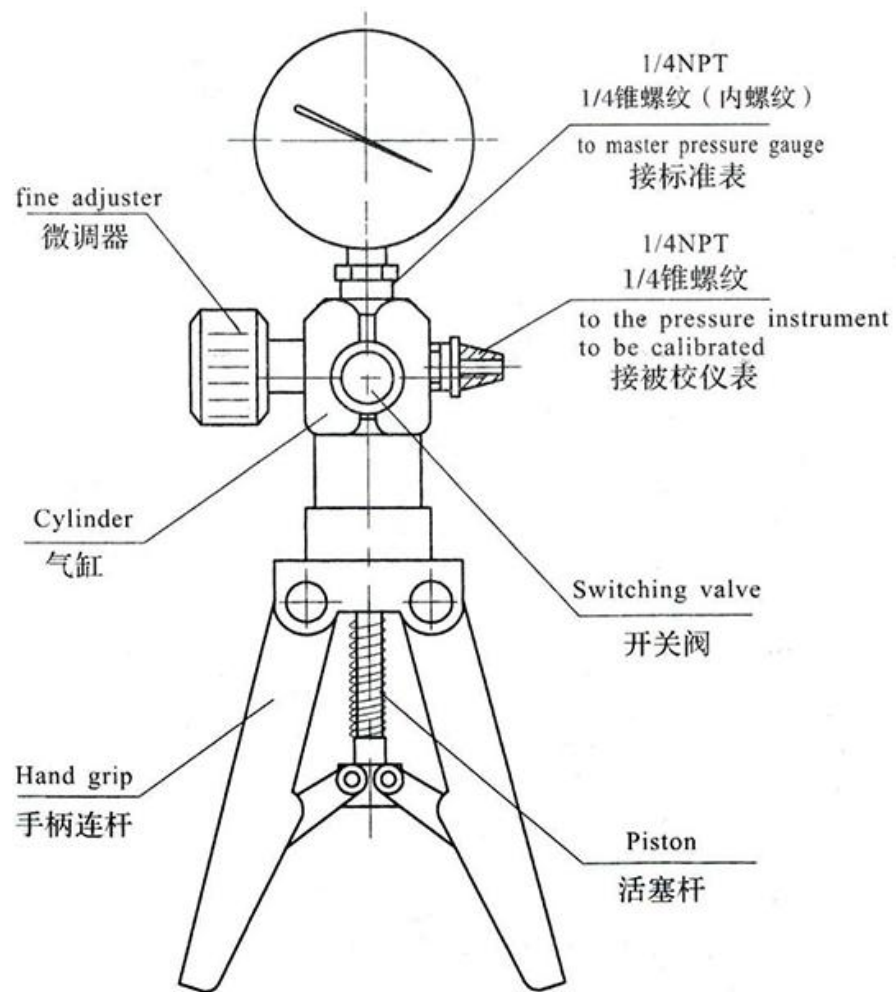

示意图

Schematic diagram